

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

**Catalog No: E-BC-K102-M**

**Specification: 48T(32 samples)/96T(80 samples)/500Assays(484 samples)**

**Measuring instrument: Microplate reader (402-407 nm)**

**Detection range: 0.41-125 mmol/L**

## **Elabscience® Hydrogen Peroxide (H<sub>2</sub>O<sub>2</sub>)**

### **Colorimetric Assay Kit**

This manual must be read attentively and completely before using this product.

If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tell: 1-832-243-6086

Fax: 1-832-243-6017

Email: [techsupport@elabscience.com](mailto:techsupport@elabscience.com)


Website: [www.elabscience.com](http://www.elabscience.com)

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

## Table of contents

<b>Assay summary .....</b>	<b>3</b>
<b>Intended use .....</b>	<b>4</b>
<b>Detection principle .....</b>	<b>4</b>
<b>Kit components &amp; storage .....</b>	<b>4</b>
<b>Materials prepared by users .....</b>	<b>5</b>
<b>Reagent preparation .....</b>	<b>5</b>
<b>Sample preparation .....</b>	<b>6</b>
<b>The key points of the assay .....</b>	<b>7</b>
<b>Operating steps .....</b>	<b>8</b>
<b>Calculation .....</b>	<b>9</b>
<b>Appendix I Performance Characteristics .....</b>	<b>10</b>
<b>Appendix II Example Analysis .....</b>	<b>12</b>
<b>Appendix III Publications .....</b>	<b>13</b>
<b>Statement .....</b>	<b>14</b>

## Assay summary

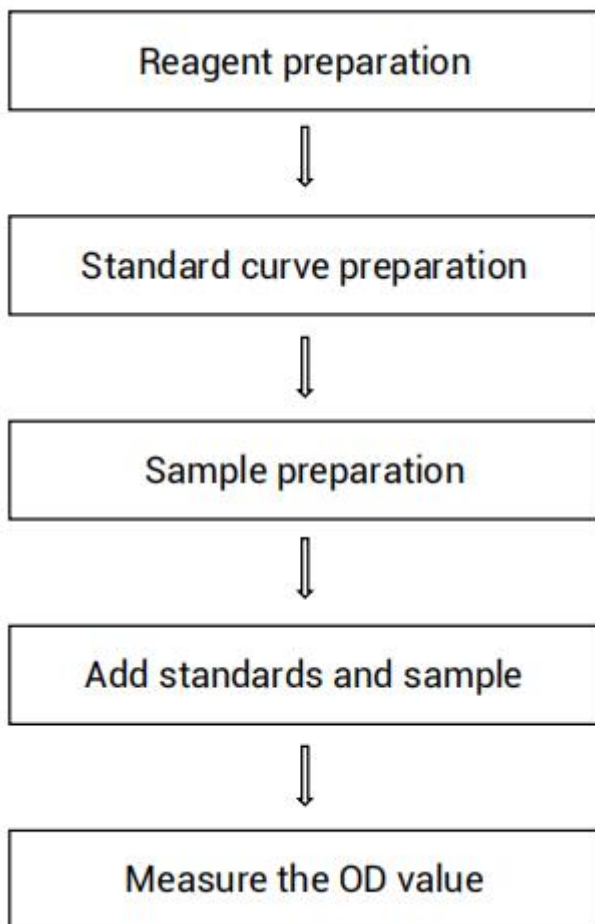

## Intended use

This kit can be used to measure the  $\text{H}_2\text{O}_2$  content in serum, plasma, urine, tissue and cells samples.

## Detection principle

Hydrogen peroxide ( $\text{H}_2\text{O}_2$ ) is a metabolic by-product of reactive oxygen species, which is not only a signal molecule in cells, but also a source of oxidative stress.  $\text{H}_2\text{O}_2$  is an important regulatory factor of eukaryotic signal transduction involved in cell proliferation, differentiation and migration. However, abnormal  $\text{H}_2\text{O}_2$  can lead to oxidative cell damage and disease, such as cancer, atherosclerosis, osteoporosis and neurodegenerative diseases.

## Kit components & storage

Item	Component	Size 1 (48 T)	Size 2 (96 T)	Size 3 (500Assays)	Storage
Reagent 1	Buffer Solution	6 mL×1 vial	12 mL×1 vial	60 mL×1 vial	2-8°C, 12 months
Reagent 2	Ammonium Molybdate Reagent	6 mL×1 vial	12 mL×1 vial	60 mL×1 vial	2-8°C, 12 months
Reagent 3	1 mol/L $\text{H}_2\text{O}_2$ Standard	1 mL×1 vial	1 mL×2 vials	10 mL×1 vial	2-8°C, 12 months
	Microplate	48 wells	96 wells	/	No requirement
	Plate Sealer	2 pieces			
	Sample Layout Sheet	1 piece			

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

## Materials prepared by users

### Instruments:

Microplate reader (402-407 nm, optimum wavelength: 405 nm),

Micropipettor, Centrifuge, Incubator, Vortex mixer

### Reagents:

Double distilled water, Normal saline (0.9% NaCl), PBS (0.01 M, pH 7.4)

## Reagent preparation

- ① Equilibrate all the reagents to room temperature before use.
- ② If precipitation occurs in buffer solution. it can be redissolved by heating in 80°C water bath before use.

- ③ The preparation of standard curve:

Always prepare a fresh set of standards. Discard working standard dilutions after use.

Dilute 1 mol/L standard solution with double distilled water to a serial concentration. The recommended dilution gradient is as follows: 0, 10, 20, 40, 60, 80, 100, 125 mmol/L. Reference is as follows:

Item	①	②	③	④	⑤	⑥	⑦	⑧
<b>Concentration (mmol/L)</b>	<b>0</b>	<b>10</b>	<b>20</b>	<b>40</b>	<b>60</b>	<b>80</b>	<b>100</b>	<b>125</b>
<b>1 mol/L standard (μL)</b>	0	10	20	40	60	80	100	125
<b>Double distilled water (μL)</b>	1000	990	980	960	940	920	900	875

## Sample preparation

### ① Sample preparation

**Serum, plasma and urine:** detect directly. If not detected on the same day, the serum or plasma can be stored at  $-80^{\circ}\text{C}$  for a month.

### **Tissue sample:**

- ① Harvest the amount of tissue needed for each assay (initial recommendation 20 mg).
- ② Wash tissue in cold PBS (0.01 M, pH 7.4).
- ③ Homogenize 20 mg tissue in 180  $\mu\text{L}$  PBS (0.01 M, pH 7.4) with a dounce homogenizer at  $4^{\circ}\text{C}$ .
- ④ Centrifuge at  $10000\times g$  for 10 min to remove insoluble material. Collect supernatant and keep it on ice for detection.
- ⑤ Meanwhile, determine the protein concentration of supernatant (E-BC-K318-M).

### **Cell (adherent or suspension) samples:**

- ① Harvest the number of cells needed for each assay (initial recommendation  $1\times 10^6$  cells).
- ② Wash cells with PBS (0.01 M, pH 7.4).
- ③ Homogenize  $1\times 10^6$  cells in 300-500  $\mu\text{L}$  PBS (0.01 M, pH 7.4) with a ultrasonic cell disruptor at  $4^{\circ}\text{C}$ .
- ④ Centrifuge at  $10000\times g$  for 10 min to remove insoluble material. Collect supernatant and keep it on ice for detection.
- ⑤ Meanwhile, determine the protein concentration of supernatant (E-BC-K318-M).

## ② Dilution of sample

The recommended dilution factor for different samples is as follows (for reference only):

Sample type	Dilution factor
Human serum	1
Rat serum	1
Mouse serum	1
Mouse plasma	1
Porcine serum	1
Human urine	1
Cell homogenate	1
10% Plant tissue homogenate	1
10% Rat heart tissue homogenate	1
10% Rat brain tissue homogenate	1
10% Rat kidney tissue homogenate	1
10% Rat liver tissue homogenate	1

Note: The diluent is normal saline (0.9% NaCl) or PBS (0.01 M, pH 7.4). For the dilution of other sample types, please do pretest to confirm the dilution factor.

## The key points of the assay

If the concentration of  $\text{H}_2\text{O}_2$  in the sample is too high, please dilute the samples appropriately. If the concentration is too low, the sampling volume of the sample should be increased, and the sampling volume of standard and double distilled water should be increased equally at the same time.

## Operating steps

- ① Add 100  $\mu\text{L}$  of buffer solution to standard well and sample well, preheat at  $37^{\circ}\text{C}$  for 10 min.
- ② Standard well: add 15  $\mu\text{L}$  of standards with different concentrations to the corresponding wells.  
Sample well: add 15  $\mu\text{L}$  of sample to the corresponding wells.
- ③ Add 100  $\mu\text{L}$  of ammonium molybdate reagent and mix fully.
- ④ Mix for 5 s with microplate reader and stand for 10 min at room temperature.
- ⑤ Measure the OD values of each well at 405 nm with microplate reader.



## Calculation

### The standard curve:

1. Average the duplicate reading for each standard.
2. Subtract the mean OD value of the blank (Standard #①) from all standard readings. This is the absolved OD value.
3. Plot the standard curve by using absolved OD value of standard and correspondent concentration as y-axis and x-axis respectively. Create the standard curve ( $y = ax + b$ ) with graph software (or EXCEL).

### The sample:

#### 1. Serum (plasma) sample and other liquid samples:

$$\text{H}_2\text{O}_2 \text{ content (mmol/L)} = (\Delta A_{405} - b) \div a \times f$$

#### 2. Tissue and cell samples:

$$\text{H}_2\text{O}_2 \text{ content (mmol/gprot)} = (\Delta A_{405} - b) \div a \div C_{pr} \times f$$

### [Note]

$\Delta A_{405}$ : Absolute OD ( $\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}$ ).

f: Dilution factor of sample before test.

$C_{pr}$ : Concentration of protein in sample, gprot/L.

## Appendix I Performance Characteristics

### 1. Parameter:

#### Intra-assay Precision

Three human serum samples were assayed in replicates of 20 to determine precision within an assay. (CV = Coefficient of Variation)

Parameters	Sample 1	Sample 2	Sample 3
Mean (mmol/L)	5.50	48.60	102.30
%CV	3.5	3.1	3.0

#### Inter-assay Precision

Three human serum samples were assayed 20 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean (mmol/L)	5.50	48.60	102.30
%CV	3.2	3.6	4.0

#### Recovery

Take three samples of high concentration, middle concentration and low concentration to test the samples of each concentration for 6 times parallelly to get the average recovery rate of 105%.

	Standard 1	Standard 2	Standard 3
Expected Conc. (mmol/L)	16.5	55.8	95
Observed Conc. (mmol/L)	17.7	58.0	98.8
Recovery rate (%)	107	104	104


#### Sensitivity

The analytical sensitivity of the assay is 0.41 mmol/L. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

## 2. Standard curve:

As the OD value of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique or temperature effects), so the standard curve and data are provided as below for reference only:

Concentration (mmol/L)	0	10	20	40	60	80	100	125
OD value	0.072	0.132	0.188	0.287	0.380	0.468	0.543	0.636
	0.076	0.134	0.184	0.293	0.384	0.460	0.545	0.634
Average OD	0.074	0.133	0.186	0.290	0.382	0.464	0.544	0.635
Absoluted OD	0	0.059	0.112	0.216	0.308	0.390	0.470	0.561

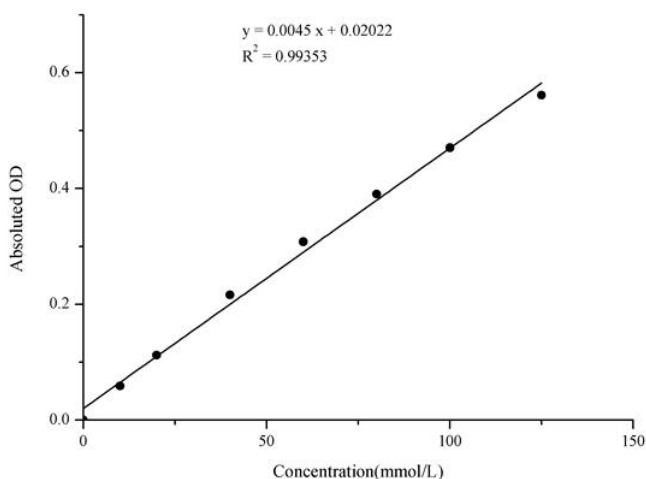

## Appendix Π Example Analysis


### Example analysis :

Take 15  $\mu\text{L}$  of human serum sample and carry the assay according to the operation steps. The results are as follows:

Standard curve:  $y = 0.0047x + 0.0223$ , the average OD value of the sample is 0.435, the average OD value of the blank is 0.075, and the calculation result is:

$$\text{H}_2\text{O}_2 \text{ content (mmol/L)} = (0.435 - 0.075 - 0.0223) \div 0.0047 \times 1 = 71.85 \text{ (mmol/L)}$$

Detect human serum, HepG2 cell homogenate (the concentration of protein in sample is 5.00 gprot/L), 10% rat kidney tissue homogenate (the concentration of protein in sample is 6.57 gprot/L), 10% epipremnum aureum tissue homogenate (the concentration of protein in sample is 0.99 gprot/L) according to the protocol, the result is as follows:

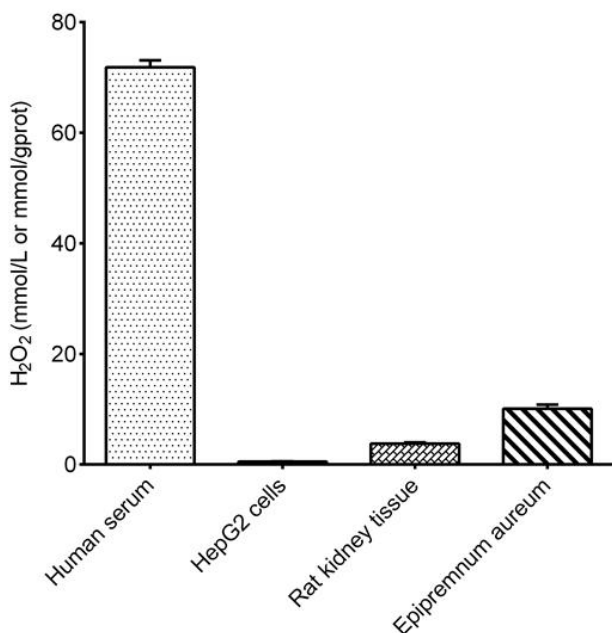

## Appendix III Publications

1. Liu H, Ji M, Qin Y, et al. Harnessing self-assembled nanoplatfrom of Dexamethasone and  $\alpha$ -linolenic acid for high-efficiency inhibition of pulmonary cytokine storm and fibrosis in mice[J]. Nano Today, 2024, 55: 102201.
  2. Du S, Zhou N, Xie G, et al. Surface-engineered triboelectric nanogenerator patches with drug loading and electrical stimulation capabilities: Toward promoting infected wounds healing[J]. Nano Energy, 2021, 85: 106004.
  3. Zhang W, Lu H, Zhang W, et al. Inflammatory microenvironment - responsive hydrogels enclosed with quorum sensing inhibitor for treating post - traumatic osteomyelitis[J]. Advanced Science, 2024, 11(20): 2307969.
  4. Zhang L, Shi W Y, Xu J Y, et al. Protective effects and mechanism of chemical-and plant-based selenocystine against cadmium-induced liver damage[J]. Journal of Hazardous Materials, 2024, 468: 133812.
  5. Li G, Zhang J, Zhang S, et al. Multifunctional nanoadjuvant-driven microenvironment modulation for enhanced photothermal immunotherapy in breast cancer[J]. Journal of Controlled Release, 2023, 362: 309-324.
- Tian J, Wang L, Hui S, et al. Cadmium accumulation regulated by a rice heavy-metal importer is harmful for host plant and leaf bacteria[J]. Journal of Advanced Research, 2023, 45: 43-57.

## Statement

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.



