

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

Catalog No: E-BC-K1105-M

Specification: 48T(32 samples)/96T(80 samples)

Measuring instrument: Microplate reader (500 nm)

Detection range: 12.60-300.00 μ mol/L

Elabscience® Biotin Colorimetric Assay Kit

This manual must be read attentively and completely before using this product.

If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tell: 1-832-243-6086

Fax: 1-832-243-6017

Email: techsupport@elabscience.com


Website: www.elabscience.com

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

Table of contents

| | |
|---|----|
| Assay summary | 3 |
| Intended use | 4 |
| Detection principle | 4 |
| Kit components & storage | 4 |
| Materials prepared by users | 5 |
| Reagent preparation | 5 |
| Sample preparation | 6 |
| Operating steps | 7 |
| Calculation | 7 |
| Appendix I Performance Characteristics | 8 |
| Statement | 10 |

Assay summary

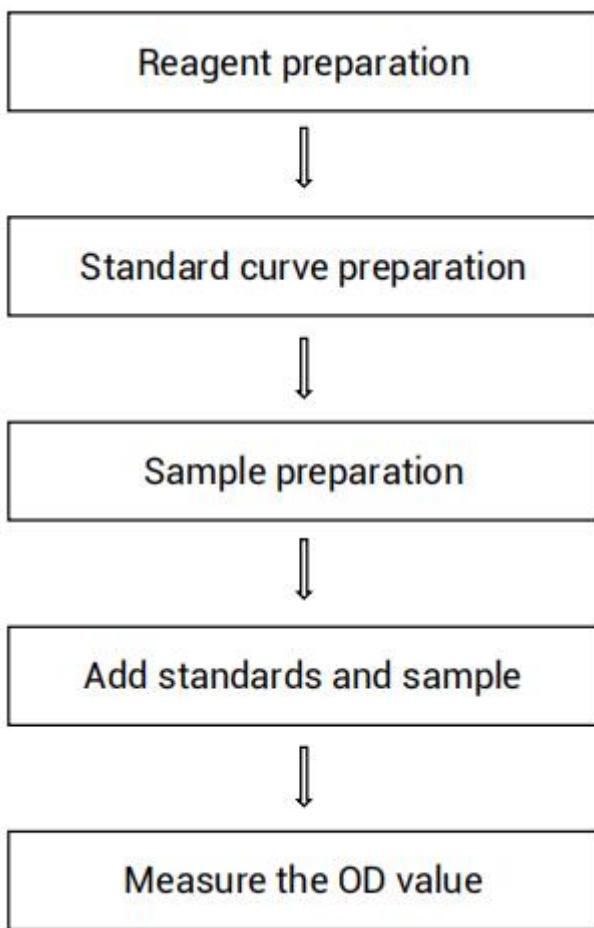

Intended use

This kit can be used to measure the biotin content of antibodies or proteins that have been biotinylated.

Detection principle

Biotin is an important biological molecule that is widely used to label antibodies or other proteins in biotinylated reactions.

The detection principle: Biotin can compete with avidin for binding to the dye, causing a decrease in the absorbance value at 500 nm, calculate the content of biotin.

Kit components & storage

| Item | Component | Size 1(48 T) | Size 2(96 T) | Storage |
|-----------|-----------------------------|------------------|------------------|---------------------------------|
| Reagent 1 | Buffer Solution | 15 mL × 1 vial | 30 mL 1vial | -20°C, 12 months, shading light |
| Reagent 2 | Substrate A | 0.02 mL × 1 vial | 0.04 mL × 1 vial | -20°C, 12 months, shading light |
| Reagent 3 | Substrate B | 0.6 mL × 1 vial | 1.2 mL × 1 vial | -20°C, 12 months, shading light |
| Reagent 4 | Alkali Reagent | 2 mL × 1 vial | 4 mL × 1 vial | -20°C, 12 months, shading light |
| Reagent 5 | 30 mmol/L Standard Solution | 0.02 mL × 1 vial | 0.02 mL × 1 vial | -20°C, 12 months, shading light |
| | Microplate | 48 wells | 96 wells | No requirement |
| | Plate Sealer | 2 pieces | | |
| | Sample Layout Sheet | 1 piece | | |

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

Materials prepared by users

Instruments:

Microplate reader (500 nm), Incubator

Reagent preparation

① Equilibrate all reagents to 25°C before use.

② The preparation of substrate A dilution solution:

Before testing, please prepare sufficient substrate A dilution solution according to the test wells. For example, prepare 100 µL of substrate A dilution solution (mix well 10 µL of alkali reagent and 90 µL of buffer solution). Aliquoted storage at -20°C for 7 days protected from light.

③ The preparation of substrate A working solution:

Before testing, please prepare sufficient substrate A working solution according to the test wells. For example, prepare 1000 µL of substrate A working solution (mix well 100 µL of substrate A and 900 µL of substrate A dilution solution, yellow and transparent is effective). Store at -20°C for 1 day protected from light.

④ The preparation of substrate B working solution:

Before testing, please prepare sufficient substrate B working solution according to the test wells. For example, prepare 200 µL of substrate B working solution (mix well 100 µL of substrate B and 100 µL of double distilled water). Aliquoted storage at -20°C for 7 days protected from light.

⑤ The preparation of reaction working solution:

For each well, prepare 40 µL of reaction working solution (mix well 20 µL of substrate A working and 20 µL of substrate B working, orange and transparent is effective). Aliquoted storage at -20°C for 1 day

protected from light.

⑥ The preparation of 300 $\mu\text{mol/L}$ standard solution:

Before testing, please prepare sufficient 300 $\mu\text{mol/L}$ standard solution.

For example, prepare 1000 μL of 300 $\mu\text{mol/L}$ standard solution (mix well 10 μL of 30 mmol/L standard solution and 990 μL of buffer solution). Aliquoted storage at -20°C for 7 days protected from light.

⑦ The preparation of standard curve:

Always prepare a fresh set of standards. Discard working standard dilutions after use.

Dilute 300 $\mu\text{mol/L}$ standard solution with buffer solution to a serial concentration. The recommended dilution gradient is as follows: 0, 60, 90, 120, 150, 180, 210, 300 $\mu\text{mol/L}$. Reference is as follows:

| Item | ① | ② | ③ | ④ | ⑤ | ⑥ | ⑦ | ⑧ |
|--|-----|-----|-----|-----|-----|-----|-----|-----|
| Concentration ($\mu\text{mol/L}$) | 0 | 60 | 90 | 120 | 150 | 180 | 210 | 300 |
| 300 $\mu\text{mol/L}$ Standard (μL) | 0 | 40 | 60 | 80 | 100 | 120 | 140 | 200 |
| Buffer Solution (μL) | 200 | 160 | 140 | 120 | 100 | 80 | 60 | 0 |

Sample preparation

Antibodies or proteins labeled with biotin: detect directly.

Operating steps

- ① Standard well: add 20 μL of standard with different concentrations into the standard wells.
Sample well: add 20 μL of sample into the sample wells.
- ② Add 40 μL of reaction working solution into each well.
- ③ Add 140 μL of buffer solution into each well.
- ④ Measure the OD values of each well at 500 nm with microplate reader.

Calculation

The standard curve:

1. Average the duplicate reading for each standard.
2. Subtract the mean OD value of the blank (Standard # ①) from all standard readings. This is the absolutized OD value.
3. Plot the standard curve by using absolutized OD value of standard and correspondent concentration as y-axis and x-axis respectively. Create the standard curve ($y = ax + b$) with graph software (or EXCEL).

The sample:

$$\text{Biotin content} = (\Delta A - b) \div a \times f$$
$$(\mu\text{mol/L})$$

[Note]

ΔA : $\text{OD}_{\text{blank}} - \text{OD}_{\text{sample}}$

f: Dilution factor of sample before test.

Appendix I Performance Characteristics

1. Parameter:

Intra-assay Precision

Three antibodies samples were assayed in replicates of 20 to determine precision within an assay (CV = Coefficient of Variation).

| Parameters | Standard 1 | Standard 2 | Standard 3 |
|---------------|------------|------------|------------|
| Mean (µmol/L) | 50.00 | 100.00 | 150.00 |
| %CV | 1.2 | 1.4 | 3.4 |

Inter-assay Precision

Three antibodies samples were assayed 20 times in duplicate by three operators to determine precision between assays.

| Parameters | Standard 1 | Standard 2 | Standard 3 |
|---------------|------------|------------|------------|
| Mean (µmol/L) | 50.00 | 100.00 | 150.00 |
| %CV | 3.5 | 4.5 | 6.0 |


Sensitivity

The analytical sensitivity of the assay is 12.60 µmol/L. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

2. Standard curve:

As the OD value of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique or temperature effects), so the standard curve and data are provided as below for reference only:

| Concentration ($\mu\text{mol/L}$) | 0 | 60 | 90 | 120 | 150 | 180 | 210 | 300 |
|--|-------|-------|-------|-------|-------|-------|-------|-------|
| OD | 0.272 | 0.240 | 0.208 | 0.195 | 0.179 | 0.145 | 0.132 | 0.072 |
| | 0.274 | 0.234 | 0.217 | 0.203 | 0.176 | 0.150 | 0.130 | 0.079 |
| Average OD | 0.273 | 0.237 | 0.213 | 0.199 | 0.178 | 0.148 | 0.131 | 0.076 |
| Absoluted OD | 0.000 | 0.036 | 0.060 | 0.074 | 0.095 | 0.125 | 0.142 | 0.197 |

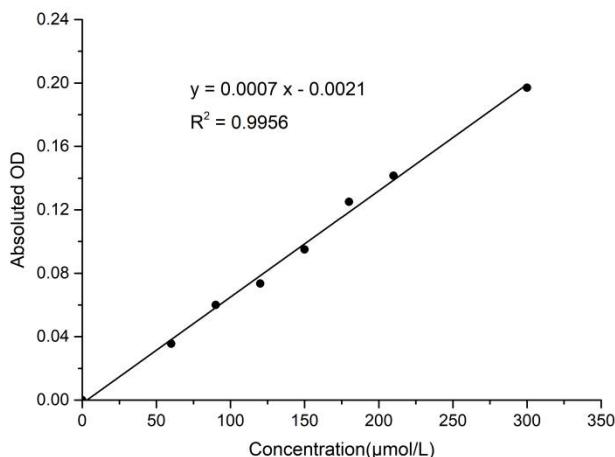

Statement

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.

