

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

**Catalog No: E-BC-K298-M**

**Specification: 48T(32 samples)/96T(80 samples)/ 500Assays(484 samples)**

**Measuring instrument: Microplate reader (530-540 nm)**

**Detection range: 2.6-100  $\mu$ mol/L**

## **Elabscience<sup>®</sup> Thiobarbituric Acid Reactants (TBARS) Colorimetric Assay Kit**

This manual must be read attentively and completely before using this product.

If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tel: 1-832-243-6086

Fax: 1-832-243-6017

Email: [techsupport@elabscience.com](mailto:techsupport@elabscience.com)


Website: [www.elabscience.com](http://www.elabscience.com)

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

## Table of contents

<b>Assay summary</b> .....	3
<b>Intended use</b> .....	4
<b>Detection principle</b> .....	4
<b>Kit components &amp; storage</b> .....	4
<b>Materials prepared by users</b> .....	5
<b>Reagent preparation</b> .....	5
<b>Sample preparation</b> .....	7
<b>The key points of the assay</b> .....	8
<b>Operating steps</b> .....	8
<b>Calculation</b> .....	9
<b>Appendix I Performance Characteristics</b> .....	10
<b>Appendix II Example Analysis</b> .....	12
<b>Appendix III Publications</b> .....	13
<b>Statement</b> .....	14

## Assay summary

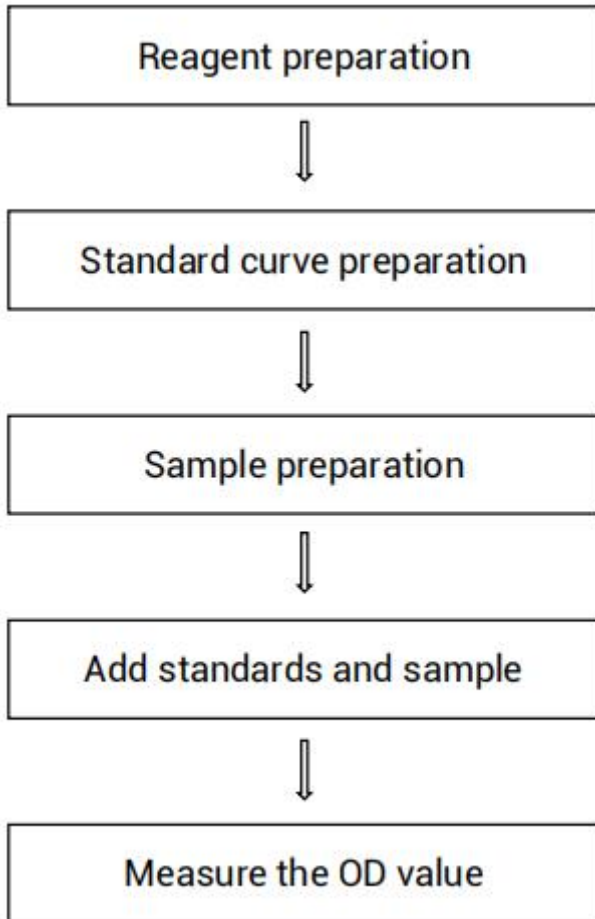


## Intended use

This kit can be used to measure TBARS concentration in serum (plasma), animal tissue samples.

## Detection principle

TBARS can react with TBA under high temperature and acid conditions to form a pink compound, the concentration of which is linearly related to the concentration of TBARS in the sample. The TBARS concentration can be calculated by measuring the OD values at 530-540 nm.

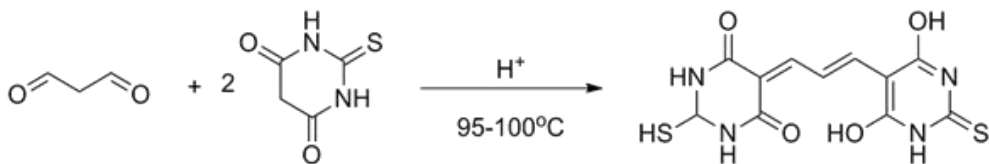

## Kit components & storage

Item	Component	Size 1(48 T)	Size 2(96 T)	Size 3 (500 Assays)	Storage
Reagent 1	Clarificant	12 mL × 1 vial	12 mL × 1 vial	60 mL × 1 vial	2-8°C, 12 months
Reagent 2	Acid Reagent	6 mL × 1 vial	12 mL × 1 vial	60 mL × 1 vial	2-8°C, 12 months
Reagent 3	TBA Reagent	Powder × 1 vial	Powder × 1 vial	Powder × 5 vials	2-8°C, 12 months shading light
Reagent 4	200 μmol/L Standard	5 mL × 1 vial	5 mL × 1 vial	15 mL × 2 vials	2-8°C, 12 months
	Microplate	96 wells		/	No requirement
	Plate Sealer	2 pieces			
	Sample Layout Sheet	1 piece			

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

## **Materials prepared by users**

### **Instruments:**

Microplate reader (530-540 nm), Vortex mixer, Micropipettor, Water bath

### **Reagents:**

Double distilled water, Acetic acid, normal saline (0.9% NaCl), PBS (0.01 M, pH 7.4)

## **Reagent preparation**

- ① Clarificant may solidify because of frozen storage (2-8°C). To re-dissolve place in a water bath (37°C) and until the clarificant looks clear. Equilibrate other reagents to room temperature before use.
- ② The preparation of acid application solution:  
Dilute 1.2 mL acid reagent with 34 mL double-distilled water. The acid application solution should be prepared on spot. Store at 2~8°C for 1 day.
- ③ The preparation of TBA application solution:  
Dissolve a vial of TBA reagent with 60 mL double distilled water (90-100°C) and mix fully. Then add 60 mL glacial acetic acid (self-prepared), mix fully and cool to room temperature. Store at 2~8°C for 1 month protected from light.

④ The preparation of chromogenic agent:

For each tube, prepare 4 mL of chromogenic agent (mix well 3 mL of acid application solution, 1 mL of TBA application solution). The chromogenic agent should be prepared on spot and it must be use out in 24 hours.

⑤ The preparation of standard curve:

Always prepare a fresh set of standards. Discard working standard dilutions after use.

Dilute 200  $\mu\text{mol/L}$  standard with double distilled water to a serial concentration. The recommended dilution gradient is as follows: 0, 5, 10, 20, 40, 60, 80, 100  $\mu\text{mol/L}$ . Reference is as follows:

Item	①	②	③	④	⑤	⑥	⑦	⑧
<b>Concentration (<math>\mu\text{mol/L}</math>)</b>	<b>0</b>	<b>5</b>	<b>10</b>	<b>20</b>	<b>40</b>	<b>60</b>	<b>80</b>	<b>100</b>
<b>200 <math>\mu\text{mol/L}</math> standard (<math>\mu\text{L}</math>)</b>	0	25	50	100	200	300	400	500
<b>Double distilled water (<math>\mu\text{L}</math>)</b>	1000	975	950	900	800	700	600	500

## Sample preparation

### ① Sample preparation

**Serum and plasma:** detect directly. If not detected on the same day, the serum or plasma can be stored at  $-80^{\circ}\text{C}$  for a month.

### **Tissue sample:**

- ① Harvest the amount of tissue needed for each assay (initial recommendation 20 mg).
- ② Wash tissue in cold PBS (0.01 M, pH 7.4).
- ③ Homogenize 20 mg tissue in 180  $\mu\text{L}$  PBS (0.01 M, pH 7.4) with a dounce homogenizer at  $4^{\circ}\text{C}$ .
- ④ Centrifuge at  $10000\times g$  for 10 minutes to remove insoluble material. Collect supernatant and keep it on ice for detection.
- ⑤ Meanwhile, determine the protein concentration of supernatant (E-BC-K318-M).

### ② Dilution of sample

The recommended dilution factor for different samples is as follows (for reference only):

Sample type	Dilution factor
Human serum	1
Rat serum	1
10% Mouse brain tissue homogenization	1
Human serum	1
Rat serum	1
10% Rat liver tissue homogenization	1

Note: The diluent is normal saline (0.9% NaCl) or PBS (0.01 M, pH 7.4). For the dilution of other sample types, please do pretest to confirm the dilution factor

## The key points of the assay

- ① The temperature of water-bath and the time of incubation should be stabilized (95-100°C, 60 min).
- ② In the incubation of 100°C water bath, the EP tube should not be closed directly. It is recommended to fasten the tube mouth with fresh-keeping film and make a small hole in the film.
- ③ The supernatant for colorimetric measurement should not contain sediment, otherwise it will affect the OD values. It is recommended to use a pipette to take the supernatant.

## Operating steps

### The measurement of samples

- ① Standard tube: Take 0.1 mL of standard solution with different concentrations into numbered 10 mL glass tubes.  
Sample tube: Take 0.1 mL of tested sample into numbered 10 mL glass tubes.
- ② Add 0.1 mL of clarificant into each tube.
- ③ Add 4 mL of chromogenic agent into each tube.
- ④ Fasten the tube mouth with fresh-keeping film, mix fully, and make a small hole in the film. Then incubate the tubes at 100°C for 60 min.
- ⑤ Cool the tubes to room temperature with running water, centrifuge the tubes at 1600×g for 10 min.
- ⑥ Take 0.25 mL the supernatant to the microplate with a micropipette (the precipitation cannot be added to the microplate).
- ⑦ Measure the OD value at 532 nm with microplate reader.

## Calculation

### The standard curve:

1. Average the duplicate reading for each standard.
2. Subtract the mean OD value of the blank (Standard #①) from all standard readings. This is the absolved OD value.
3. Plot the standard curve by using absolved OD value of standard and correspondent concentration as y-axis and x-axis respectively.  
Create the standard curve ( $y = ax + b$ ) with graph software (or EXCEL).

### The sample:

#### 1. Serum (plasma) sample:

$$\text{TABRS} \begin{matrix} \text{(\mu mol/L)} \end{matrix} = (\Delta A - b) \div a \times f$$

#### 2. Tissue sample:

$$\text{TABRS} \begin{matrix} \text{(\mu mol/gprot)} \end{matrix} = (\Delta A - b) \div a \times f \div C_{pr}$$

[Note]

f: Dilution factor of sample before test.

$C_{pr}$ : Concentration of protein in sample (gprot/L)

$\Delta A$ : Absolute OD ( $OD_{\text{Sample}} - OD_{\text{Blank}}$ ).

## Appendix I Performance Characteristics

### 1. Parameter:

#### Intra-assay Precision

Three human serum samples were assayed in replicates of 20 to determine precision within an assay. (CV = Coefficient of Variation)

Parameters	Sample 1	Sample 2	Sample 3
Mean ( $\mu\text{mol/L}$ )	5.90	25.70	76.50
%CV	4.5	4.2	4.2

#### Inter-assay Precision

Three human serum samples were assayed 20 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean ( $\mu\text{mol/L}$ )	5.90	25.70	76.50
%CV	6.8	7.2	7.3

#### Recovery

Take three samples of high concentration, middle concentration and low concentration to test the samples of each concentration for 6 times parallelly to get the average recovery rate of 101%.

	Standard 1	Standard 2	Standard 3
Expected Conc. ( $\mu\text{mol/L}$ )	8.4	32.5	67.5
Observed Conc. ( $\mu\text{mol/L}$ )	8.5	32.0	69.7
recovery rate (%)	101	98.5	103.2


#### Sensitivity

The analytical sensitivity of the assay is 0.85  $\mu\text{mol/L}$ . This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

## 2. Standard curve:

As the OD value of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique or temperature effects), so the standard curve and data are provided as below for reference only:

Concentration (μmol/L)	0	5	10	20	40	60	80	100
Average OD	0.045	0.064	0.085	0.126	0.206	0.287	0.361	0.434
Absoluted OD	0	0.019	0.041	0.081	0.161	0.242	0.316	0.390

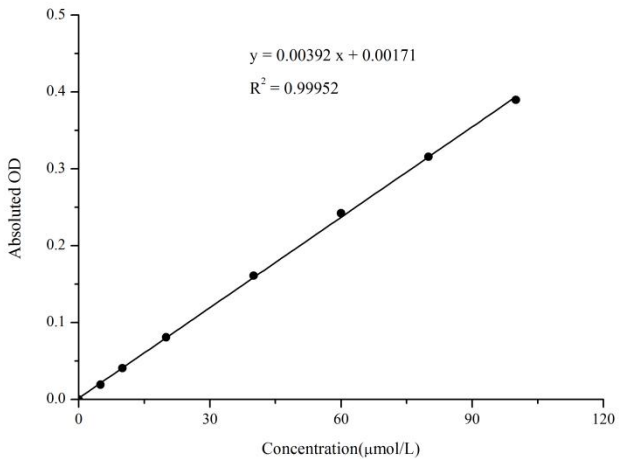

## Appendix Π Example Analysis


### Example analysis :

For mouse liver tissue, take 0.1 mL of 10% mouse tissue homogenate, carry the assay according to the operation steps. The results are as follows:

standard curve:  $y = 0.0038x - 0.0013$ , the average OD value of the sample well is 0.106, the average OD value of the blank well is 0.047, the concentration of protein in sample is 15.18 gprot/L, and the calculation result is:

$$\text{TBARS content } (\mu\text{mol/gprot}) = (0.106 - 0.047 + 0.0013) \div 0.0038 \div 15.15 = 1.05 \mu\text{mol/gprot}$$

Detect rat serum, rat plasma, mouse liver tissue (the concentration of protein in 10% tissue homogenate is 15.18 gprot/L), mouse heart tissue (the concentration of protein in 10% tissue homogenate is 5.55 gprot/L) according to the protocol, the result is as follows:

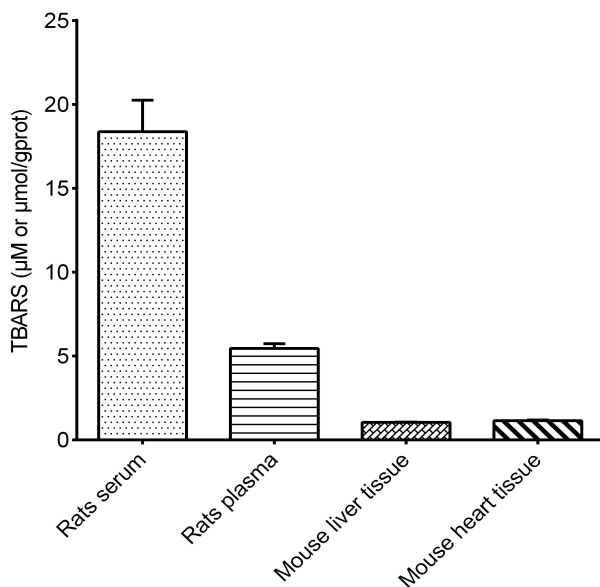

## Appendix III Publications

1. Shi C, Jia L, Tao H, et al. Fortification of cassava starch edible films with Litsea cubeba essential oil for chicken meat preservation[J]. International journal of biological macromolecules, 276 (Pt2)2): 133920 [2025-03-03]. DOI: 10.1016/j.ijbiomac.2024.133920.
2. Cui H, Yang Y, Aziz T, et al. Exploring the potential of chlorogenic acid/chitosan nanoparticle-loaded edible films with photodynamic technology for Mongolian cheese application[J]. International Journal of Biological Macromolecules, 2024, 279: 135091.
3. Shi C , Jia L , Tao H ,et al.Effects of guar gum/chitosan edible films functionalized with citronellal/HP $\beta$ CD inclusion complex on Harbin red sausage preservation[J].International Journal of Biological Macromolecules, 2024, 282(Part6):15. DOI:10.1016/j.ijbiomac.2024.137312.
4. Parn K W, Ling W C, Chin J H, et al. Safety and efficacy of dietary epigallocatechin gallate supplementation in attenuating hypertension via its modulatory activities on the intrarenal renin–angiotensin system in spontaneously hypertensive rats[J]. Nutrients, 2022, 14(21): 4605.
5. Khongwichit S, Swangphon P, Nanakorn N, et al. A simple aptamer/gold nanoparticle aggregation-based colorimetric assay for oxidized low-density lipoprotein determination[J]. Talanta, 2023, 254: 124199.
6. Kim M J, Chilakala R, Jo H G,et al. Anti-Obesity and Anti-Hyperglycemic Effects of[J]. International journal of molecular sciences, 2022, 23(7). DOI:10.3390/ijms23074015.

## Statement

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.



