

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

**Catalog No: E-BC-K284-S**

**Specification: 50 Assays(36 samples)/ 100 Assays(86 samples)**

**/ 500 Assays (486 samples)**

**Measuring instrument: Spectrophotometry (510 nm)**

**Detection range: 0.315-150 µg/mL**

## **Elabscience® Plant Flavonoids Colorimetric Assay Kit**

This manual must be read attentively and completely before using this product.

If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tell: 1-832-243-6086

Fax: 1-832-243-6017

Email: [techsupport@elabscience.com](mailto:techsupport@elabscience.com)


Website: [www.elabscience.com](http://www.elabscience.com)

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

## Table of contents

<b>Assay summary .....</b>	<b>3</b>
<b>Intended use .....</b>	<b>4</b>
<b>Detection principle .....</b>	<b>4</b>
<b>Kit components &amp; storage .....</b>	<b>4</b>
<b>Materials prepared by users .....</b>	<b>4</b>
<b>Reagent preparation .....</b>	<b>5</b>
<b>Sample preparation .....</b>	<b>6</b>
<b>Operating steps .....</b>	<b>7</b>
<b>Calculation .....</b>	<b>8</b>
<b>Appendix I Performance Characteristics .....</b>	<b>9</b>
<b>Appendix II Example Analysis .....</b>	<b>11</b>
<b>Statement .....</b>	<b>12</b>

## Assay summary

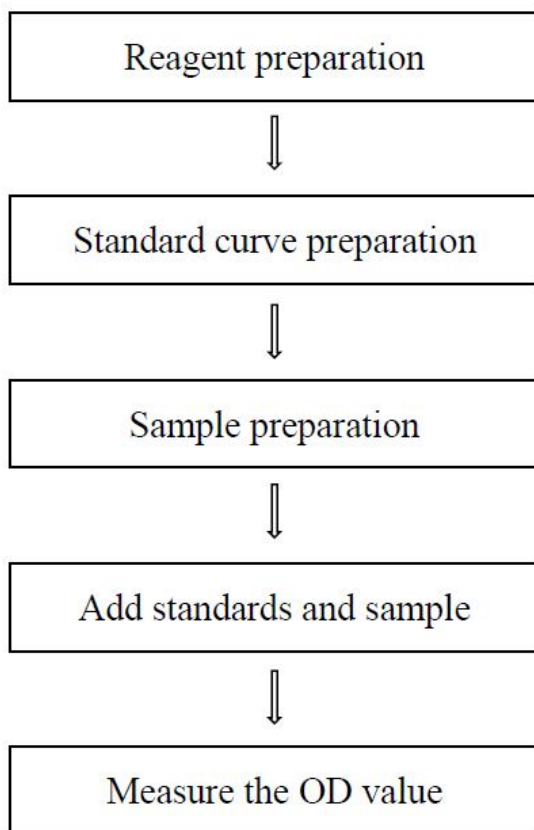

## Intended use

This kit can be used to measure the flavonoids content in plant tissue samples.

## Detection principle

In alkaline nitrite solution, flavonoids form red complex with aluminum ion. The flavonoid content of the sample can be calculated by measuring the absorbance of the sample extract at 510 nm.

## Kit components & storage

Item	Component	Size 1 (50 assays)	Size 2 (100 assays)	Size 3 (500 assays)	Storage
Reagent 1	1 mg/mL Standard	1 mL × 1 vial	2 mL × 1 vial	10 mL × 1 vial	2-8°C, 12 months
Reagent 2	Saline Solution	2 mL × 1 vial	4 mL × 1 vial	20 mL × 1 vial	2-8°C, 12 months
Reagent 3	Aluminium Reagent	2 mL × 1 vial	4 mL × 1 vial	20 mL × 1 vial	2-8°C, 12 months
Reagent 4	Alkali Reagent	25 mL×1 vial	50 mL×1 vial	50 mL × 5 vials	2-8°C, 12 months

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

## Materials prepared by users

### Instruments:

UV-visible Spectrophotometer (510 nm), Vortex mixer, Vacuum dryer, Ultrasonic cell grinder, crusher

## Reagents:

Double distilled water, 60% ethanol

## Reagent preparation

① Equilibrate all reagents to room temperature before use.

② The preparation of standard curve:

Always prepare a fresh set of standards. Discard working standard dilutions after use.

Dilute 1 mg/mL standard solution with double distilled water to a serial concentration. The recommended dilution gradient is as follows: 0, 20, 60, 80, 100, 120, 150  $\mu\text{g/mL}$ . Reference is as follows:

Item	①	②	③	④	⑤	⑥	⑦
<b>Concentration (<math>\mu\text{g/mL}</math>)</b>	<b>0</b>	<b>20</b>	<b>60</b>	<b>80</b>	<b>100</b>	<b>120</b>	<b>150</b>
<b>1 mg/mL standard (<math>\mu\text{L}</math>)</b>	0	24	72	96	120	144	180
<b>Absolute ethanol (<math>\mu\text{L}</math>)</b>	1200	1176	1128	1104	1080	1056	1020

## Sample preparation

### ① Sample preparation

**Drying and crushing of plant tissues:** Weigh 5-10 g fresh plant tissue and wash with distilled water, absorb moisture on the surface of tissue with filter paper, then put in a vacuum dryer and dry to constant weight at 80°C. Crush the sample and filter over 40 mesh screen, sealed at room temperature.

**Extraction of Plant tissue:** Accurately weigh 0.02 g sample in step 1, add 2 mL of 60% alcohol (self-prepared), then shake at 60°C for 2 hours with constant temperature shaking incubator. Centrifuge at 1500×g for 10 min, then take the supernatant for detection. Or treat the sample with ultrasonic cell disruptor (power: 300 W, 3 seconds/time, interval for 4 seconds, repeat for 30 min), then centrifuge at 10000×g for 10 min, then take the supernatant for detection.

### ② Dilution of sample

The recommended dilution factor for different samples is as follows (for reference only):

Sample type	Dilution factor
Camphor leaves tissue homogenization	8-15
Carrot tissue homogenization	2-5
Green pepper tissue homogenization	1

Note: The diluent is 60% ethanol. For the dilution of other sample types, please do pretest to confirm the dilution factor

## Operating steps

- ① Standard tube: Add 0.54 mL of standard solution with different concentrations into the 2 mL EP tubes.  
Sample tube: Add 0.54 mL of sample into a 2 mL EP tube.
- ② Add 0.03 mL of saline solution into each tube, oscillate fully and stand for 5 min at room temperature.
- ③ Add 0.03 mL of aluminium reagent into each tube, oscillate fully and stand for 5 min at room temperature.
- ④ Add 0.4 mL of alkali reagent into each tube, oscillate fully and stand for 15 min at room temperature.
- ⑤ Set the spectrophotometer to zero with double distilled water and measure the OD values of each tube at 510 nm with 0.5 cm optical path cuvette.

## Calculation

### The standard curve:

1. Average the duplicate reading for each standard.
2. Subtract the mean OD value of the blank (Standard #①) from all standard readings. This is the absolved OD value.
3. Plot the standard curve by using absolved OD value of standard and correspondent concentration as y-axis and x-axis respectively. Create the standard curve ( $y = ax + b$ ) with graph software (or EXCEL).

### The sample:

$$\text{Flavonoids content (mg/g tissue)} = (\Delta A_{510} - b) \div a \times V \div W \div 1000 \times f$$

[Note]

$\Delta A_{510}$ :  $OD_{\text{sample}} - OD_{\text{blank}}$

V: the volume of 60% alcohol in the pretreatment of sample, 2 mL.

W: weight of sample, 0.02 g.

1000: unit conversion ( $\mu\text{g} \rightarrow \text{mg}$ ).

f: the dilution multiple of tested samples.



## Appendix I Performance Characteristics

### 1. Parameter:

#### Intra-assay Precision

Three human serum samples were assayed in replicates of 20 to determine precision within an assay. ( CV = Coefficient of Variation)

Parameters	Sample 1	Sample 2	Sample 3
Mean ( $\mu\text{g/mL}$ )	5.80	75.60	126.90
%CV	2.3	1.8	1.6

#### Inter-assay Precision

Three human serum samples were assayed 20 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean ( $\mu\text{g/mL}$ )	5.80	75.60	126.90
%CV	1.8	2.3	2.5

#### Recovery

Take three samples of high concentration, middle concentration and low concentration to test the samples of each concentration for 6 times parallelly to get the average recovery rate of 98%.

	Standard 1	Standard 2	Standard 3
Expected Conc. ( $\mu\text{g/mL}$ )	45.5	95.5	114
Observed Conc. ( $\mu\text{g/mL}$ )	46.0	91.7	110.6
recovery rate (%)	101	96	97


#### Sensitivity

The analytical sensitivity of the assay is  $0.315 \mu\text{g/mL}$ . This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

**2. Standard curve:**

As the OD value of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique or temperature effects), so the standard curve and data are provided as below for reference only:

Concentration (µg/mL)	0	20	60	80	100	120	150
Average OD	0.001	0.057	0.169	0.223	0.278	0.326	0.410
Absoluted OD	0	0.056	0.168	0.222	0.277	0.325	0.409

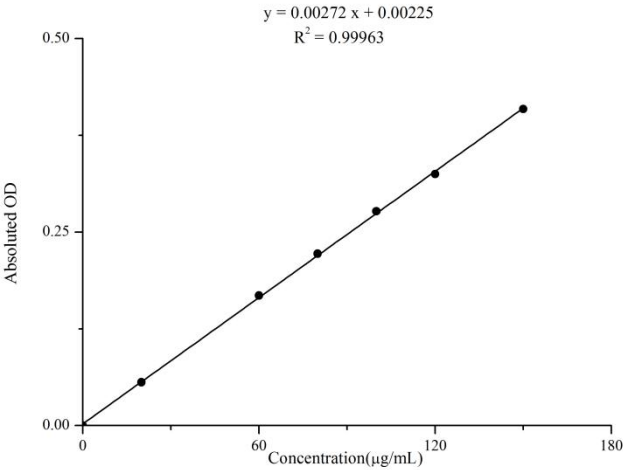

## Appendix II Example Analysis


### Example analysis:

For daucus carota tissue, take the sample pretreated and dilute the sample with 60% ethanol for 2 times, take 0.54 mL of diluted sample, and carry the assay according to the operation steps. The results are as follows:

standard curve:  $y = 0.0029x + 0.0008$  ( $R^2=0.9993$ ), the average OD value of the sample well is 0.203, the average OD value of the blank well is 0.0025, and the calculation result is:

$$\begin{aligned}\text{Flavonoids content (mg/g tissue)} &= (0.203 - 0.0025 - 0.0008) \div 0.0029 \times 2 \div 0.02 \div 1000 \times 2 \\ &= 13.77 \text{ mg/g tissue}\end{aligned}$$

Detect camphor leaf (dilute for 10 times), daucus carota (dilute for 2 times), green pepper according to the protocol, the result is as follows:

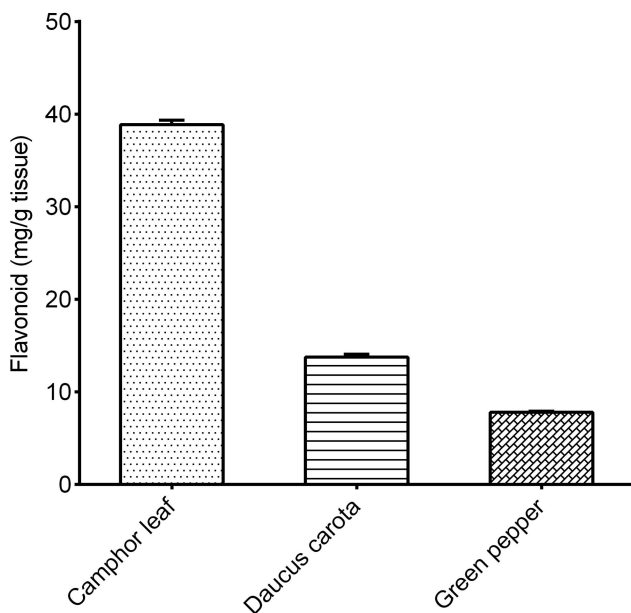

## Statement

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.