

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

**Catalog No: E-BC-K013-M**

**Specification: 48T(16 samples)/96T(40 samples)**

**Measuring instrument: Microplate reader (715 nm)**

**Detection range: 0.15-1.5 mmol/L**

## **Elabscience® Non-esterified Free Fatty Acids (NEFA/FFA) Colorimetric Assay Kit**

This manual must be read attentively and completely before using this product.

If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tel: 1-832-243-6086

Fax: 1-832-243-6017

Email: [techsupport@elabscience.com](mailto:techsupport@elabscience.com)


Website: [www.elabscience.com](http://www.elabscience.com)

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

## Table of contents

<b>Assay summary</b> .....	3
<b>Intended use</b> .....	4
<b>Detection principle</b> .....	4
<b>Kit components &amp; storage</b> .....	4
<b>Materials prepared by users</b> .....	5
<b>Reagent preparation</b> .....	5
<b>Sample preparation</b> .....	6
<b>The key points of the assay</b> .....	6
<b>Operating steps</b> .....	7
<b>Calculation</b> .....	8
<b>Appendix I Performance Characteristics</b> .....	9
<b>Appendix II Example Analysis</b> .....	11
<b>Appendix III Publications</b> .....	12
<b>Statement</b> .....	13

## Assay summary

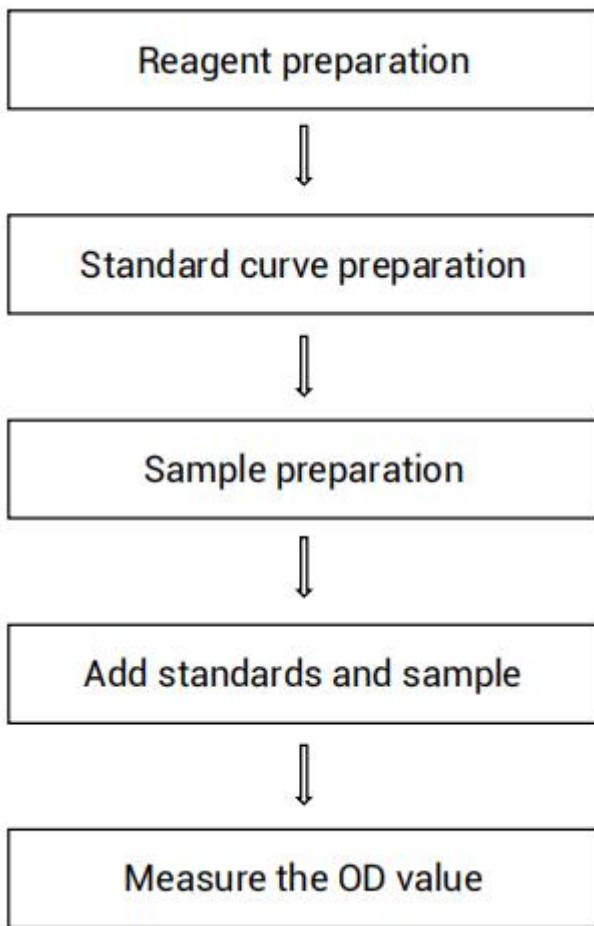

## Intended use

This kit can be used to measure non-esterified free fatty acids (NEFA) content in animal tissue samples.

## Detection principle

Under the condition of weak acidity, NEFA react with nantokite to form copper soap, which has a specific absorption peak at 715 nm. The content of NEFA can be calculated indirectly by measuring the OD value at 715 nm.

## Kit components & storage

Item	Component	Size 1(48 T)	Size 2(96 T)	Storage
Reagent 1	Extracting Solution	60 mL ×1 vial	60 mL × 2 vials	2-8°C, 12 months
Reagent 2	10 mmol/L Palmitic Acid Standard	1 mL ×1 vial	1 mL × 2 vials	2-8°C, 12 months
Reagent 3	Control Solution	6 mL ×1 vial	12 mL × 1 vial	2-8°C, 12 months
Reagent 4	Reaction Solution	10 mL ×1 vial	20 mL × 1 vial	2-8°C, 12 months
	Microplate	48 wells	96 wells	No requirement
	Plate Sealer	2 pieces		
	Sample Layout Sheet	1 piece		

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

## Materials prepared by users

### Instruments:

Microplate reader(690-730 nm, optimum wavelength: 715 nm),

Micropipettor, Vortex mixer

## Reagent preparation

① Equilibrate other reagents to room temperature before use.

② The preparation of standard curve:

Always prepare a fresh set of standards. Discard working standard dilutions after use.

Dilute 10 mmol/L standard solution with extracting solution to a serial concentration. The recommended dilution gradient is as follows: 0, 0.3, 0.4, 0.6, 0.9, 1, 1.2, 1.5 mmol/L. Reference is as follows:

Item	①	②	③	④	⑤	⑥	⑦	⑧
Concentration (mmol/L)	0	0.3	0.4	0.6	0.9	1.0	1.2	1.5
10 mmol/L standard (μL)	0	45	60	90	135	150	180	225
Extracting solution (μL)	1500	1455	1440	1410	1365	1350	1320	1275

## **Sample preparation**

### **① Sample preparation**

#### **Tissue sample:**

- ① Harvest the amount of tissue needed for each assay (initial recommendation 100 mg).
- ② Wash tissue in cold PBS (0.01 M, pH 7.4).
- ③ Homogenize 100 mg tissue in 1200  $\mu$ L extracting solution with a dounce homogenizer at 4°C.
- ④ Oscillate at 4°C for 2 hours to extract the NEFA.
- ⑤ Centrifuge at 10000 $\times$ g for 10 min at 4°C to remove insoluble material. Collect supernatant and keep it on ice for detection.

### **② Dilution of sample**

The recommended dilution factor for different samples is as follows (for reference only):

Sample type	Dilution factor
Rat liver tissue homogenate	1
Rat heart tissue homogenate	1
Rat kidney tissue homogenate	1
Mouse liver tissue homogenate	1

Note: The diluent is extracting solution. For the dilution of other sample types, please do pretest to confirm the dilution factor

## **The key points of the assay**

- ① The samples should be fresh collected and detect within 24 hours.
- ② The supernatant after centrifugation must be clarified for the pretreatment of tissue samples. Otherwise take the turbid supernatant to another centrifuge tube and centrifuge again.
- ③ The reagent has a pungent smell. Please operate in the draught cupboard.

## Operating steps

- ① Standard tube: add 0.5 mL of standards with different concentrations into the standard tubes, and add 0.25 mL reaction solution.  
Control tube: add 0.5 mL of supernatant of sample and 0.25 mL of control solution into the control tubes.  
Sample tube: add 0.5 mL of supernatant of sample and 0.25 mL of reaction solution into the sample tubes.
- ② Oscillate for 3 min and stand at room temperature for 3 min.
- ③ Take 0.3 mL of the upper layer liquid to micro-plate and measure the OD value at 715 nm with microplate reader.

## Calculation

### The standard curve:

1. Average the duplicate reading for each standard.
2. Subtract the mean OD value of the blank (Standard # ①) from all standard readings. This is the absolated OD value.
3. Plot the standard curve by using absolated OD value of standard and correspondent concentration as y-axis and x-axis respectively. Create the standard curve ( $y = ax + b$ ) with graph software (or EXCEL).

### The sample:

#### Tissue sample:

$$\text{NEFA}(\mu\text{mol/g}) = (\Delta A_{715} - b) \div a \times \frac{V_1}{m} \times f$$

#### [Note]

$\Delta A_{715}$ : Absoluted OD value,  $OD_{\text{Sample}} - OD_{\text{Control}}$ .

m: The fresh weight of tissue sample, 0.1 g.

$V_1$ : The volume of Reagent 1 added during the pretreatment of tissue sample, 1.2 mL.

f: Dilution factor of sample before test.

## Appendix I Performance Characteristics

### 1. Parameter:

#### Intra-assay Precision

Three rat liver samples were assayed in replicates of 20 to determine precision within an assay (CV = Coefficient of Variation).

Parameters	Sample 1	Sample 2	Sample 3
Mean (mmol/L)	0.35	0.70	1.20
%CV	3.5	3.1	3.3

#### Inter-assay Precision

Three rat liver samples were assayed 20 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean(mmol/L)	0.35	0.70	1.20
%CV	5.2	5.4	4.7

#### Recovery

Take three samples of high concentration, middle concentration and low concentration to test the samples of each concentration for 6 times parallelly to get the average recovery rate of 101%.

	Standard 1	Standard 2	Standard 3
Expected Conc. (mmol/L)	0.35	0.8	1.1
Observed Conc. (mmol/L)	0.4	0.8	1.1
Recovery rate (%)	103	99	101


#### Sensitivity

The analytical sensitivity of the assay is 0.15 mmol/L NEFA. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

## 2. Standard curve:

As the OD value of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique or temperature effects), so the standard curve and data are provided as below for reference only:

Concentration (mmol/L)	0	0.3	0.4	0.6	0.9	1	1.2	1.5
Average OD	0.043	0.067	0.075	0.091	0.126	0.132	0.15	0.178
Absoluted OD	0	0.024	0.032	0.048	0.083	0.089	0.107	0.135

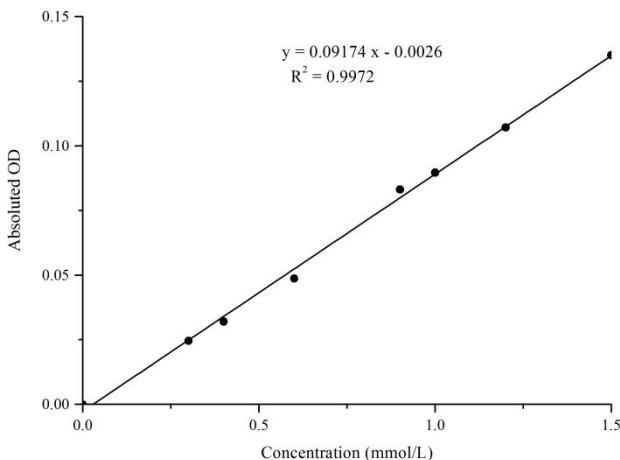

## Appendix Π Example Analysis


### Example analysis:

For rat liver tissue, take 0.1 g of rat liver tissue, add 1.2 mL extracting solution, oscillate at 4 °C for 2 hours to extract the NEFA, centrifuge at 10000×g for 10 min, dilute the supernatant with extracting solution for 3 times, and carry the assay according to the operation steps. The results are as follows:

Standard curve:  $y = 0.09174 x - 0.0026$ , the average OD value of the sample tube is 0.108, the average OD value of the control tube is 0.049, and the calculation result is:

$$\text{NEFA content} = (0.108 - 0.049 + 0.0026) \div 0.09174 \times \frac{1.2}{0.1} \times 3 = 24.17 \text{ } \mu\text{mol/g}$$

Detect rat heart tissue ( $m=0.1$  g,  $V_1=1.2$  mL), rat liver tissue ( $m=0.1$  g,  $V_1=1.2$  mL), rat kidney tissue ( $m=0.1$  g,  $V_1=1.2$  mL) according to the protocol, the result is as follows:

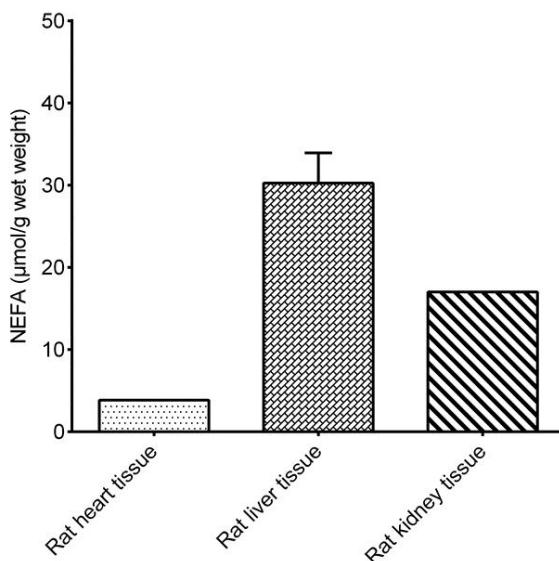

### Appendix III Publications

1. Bian Z , Xu C , Wang X ,et al.TRIM65/NF2/YAP1 Signaling Coordinately Orchestrates Metabolic and Immune Advantages in Hepatocellular Carcinoma[J].Advanced Science, 2024, 11(35).DOI:10.1002/advs.202402578.
2. Zhang X , Chen T , Li Z ,et al.NORAD exacerbates metabolic dysfunction-associated steatotic liver disease development via the miR-511-3p/Rock2 axis and inhibits ubiquitin-mediated degradation of ROCK2[J].Metabolism, 2025, 164.DOI:10.1016/j.metabol.2024.156111.
3. Lin D , Fu X , Li B ,et al.Integrating untargeted and oxylipins-targeted metabolomics to reveal the anti-obesity and hypolipidemic mechanism of conjugated linoleic acid in high-fat diet rats[J].Journal of Functional Foods, 2024, 116.DOI:10.1016/j.jff.2024.106182.
4. Kang C , Xiao Q , Wang X ,et al.Chlormequat chloride induces hepatic steatosis by promoting mTOR/SREBP1 mediated lipogenesis via AMPK inhibition[J].Food and chemical toxicology : an international journal published for the British Industrial Biological Research Association, 190:114790[2025-04-22].DOI:10.1016/j.fct.2024.114790.
5. Cai X , Zhang Q , Wang J ,et al.Novel Dual PPAR  $\delta/\gamma$  Partial Agonist Induces Hepatic Lipid Accumulation through Direct Binding and Inhibition of AKT1 Phosphorylation, Mediating CD36 Upregulation[J].Chemical Research in Toxicology, 2024, 37(9):14.DOI:10.1021/acs.chemrestox.4c00268.
6. Fingerhut M A , Henrich L , Lauber C ,et al.Characterization of a GDS(L)-like hydrolase from Pleurotus sapidus with an unusual SGNH motif[J].AMB Express, 2024, 14(1):1-14.DOI:10.1186/s13568-024-01752-x.

## **Statement**

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.





