

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

Catalog No: E-BC-K136-M

Specification: 48T(24 samples)/96T(48 samples)/ 500Assays(250 samples)

Measuring instrument: Microplate reader (500-520 nm)

Detection range: 0.62-190.43 U/mL

Elabscience® Total Antioxidant Capacity (T-AOC)

Colorimetric Assay Kit

This manual must be read attentively and completely before using this product.

If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tel: 1-832-243-6086

Fax: 1-832-243-6017

Email: techsupport@elabscience.com


Website: www.elabscience.com

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

Table of contents

Assay summary	3
Intended use	4
Detection principle	4
Kit components & storage	4
Materials prepared by users	5
Reagent preparation	5
Sample preparation	6
The key points of the assay	7
Operating steps	8
Calculation	10
Appendix I Performance Characteristics	11
Appendix II Example Analysis	12
Appendix III Publications	13
Statement	14

Assay summary

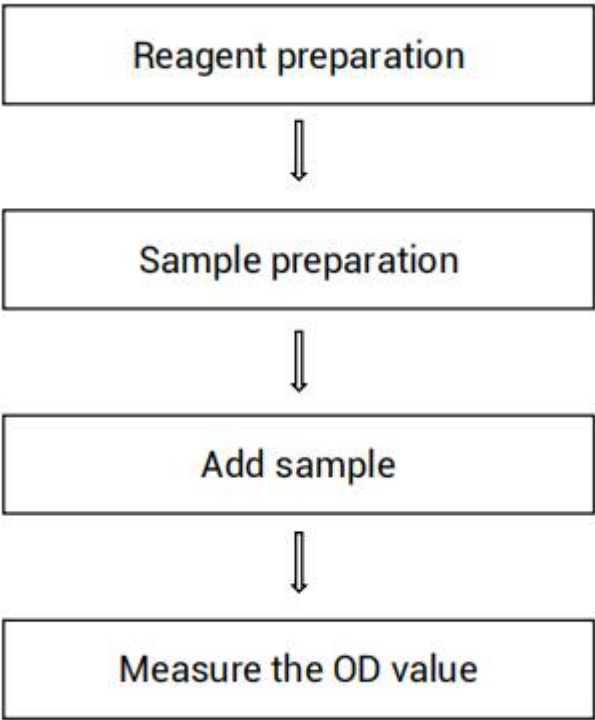

Intended use

The kit is used for the determination of total antioxidant capacity (T-AOC) in serum, plasma, whole blood, tissue, cell and culture supernatant samples.

Detection principle

A variety of antioxidant macromolecules, antioxidant molecules and enzymes in a system can eliminate all kinds of reactive oxygen species and prevent oxidative stress induced by reactive oxygen species. The total level reflect the total antioxidant capacity in the system. Many antioxidants in the body can reduce Fe^{3+} to Fe^{2+} and Fe^{2+} can form stable complexes with phenanthroline substance. The antioxidant capacity (T-AOC) can be calculated by measuring the absorbance at 520 nm.

Kit components & storage

Item	Component	Size 1(48 T)	Size 2(96 T)	Size 3 (500Assays)	Storage
Reagent 1	Buffer Solution	6 mL×1 vial	12 mL × 1 vial	60 mL×1 vial	2-8°C, 12 months
Reagent 2	Chromogenic Agent	Powder×1 vial	Powder×2 vials	Powder×10 vials	2-8°C, 12 months, shading light
Reagent 3	Ferric Salt Stock Solution	0.2 mL×1 vial	0.4 mL×1 vial	2 mL×1 vial	2-8°C, 12 months, shading light
Reagent 4	Ferric Salt Diluent	4 mL×1 vial	8 mL×1 vial	40 mL×1 vial	2-8°C, 12 months
Reagent 5	Stop Solution	1.25 mL×1 vial	1.25 mL×2 vials	12.5 mL×1 vial	2-8°C, 12 months
Reagent 6	Clarificant	1.25 mL×1 vial	1.25 mL×2 vials	12.5 mL×1 vial	2-8°C, 12 months
	Microplate	48 wells	96 wells	/	No requirement
	Plate Sealer	2 pieces			

	Sample Layout Sheet	1 piece		
--	------------------------	---------	--	--

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

Materials prepared by users

Instruments:

Microplate reader (500-520 nm, optimum wavelength: 520 nm),
Micropipettor, Centrifuge, Incubator, Vortex mixer

Reagents:

Double distilled water, Normal saline (0.9% NaCl), PBS (0.01 M, pH 7.4)

Reagent preparation

- ① Equilibrate all the reagents to room temperature before use.
- ② The preparation of chromogenic working solution:
Dissolve one vial of chromogenic agent with 20 mL of double distilled water, it can be dissolved by incubating in 80-90°C water bath and used after cooling to room temperature. Store at 2-8°C for 7 days.
- ③ The preparation of ferric salt working solution:
Before testing, please prepare sufficient ferric salt working solution according to the test wells. For example, prepare 100 µL of ferric salt working solution (mix well mix well 5 µL of ferric salt stock solution and 95 µL of ferric salt diluent). The ferric salt working solution should be prepared on spot and protect from light. Store at 2-8°C for 2 days.
- ④ Clarificant will be freeze in cold weather, dissolve by incubating in 37°C water bath until clarification before experiment.

Sample preparation

① Sample preparation

Serum, plasma and whole blood: detect directly. If not detected on the same day, the serum, plasma or whole blood can be stored at -80°C for a month.

Cell culture supernatant: Detect the cell culture supernatant directly. If there is turbidity, centrifuge at 3100 g for 10 min, take the supernatant and preserve it on ice for detection. If not detected on the same day, the cell culture supernatant can be stored at -80°C for a month.

Tissue sample:

- ① Harvest the amount of tissue needed for each assay (initial recommendation 20 mg).
- ② Wash tissue in cold PBS (0.01 M, pH 7.4).
- ③ Homogenize 20 mg tissue in 180 μ L PBS(0.01 M, pH 7.4) with a dounce homogenizer at 4°C.
- ④ Centrifuge at 10000 \times g for 10 min to remove insoluble material. Collect supernatant and keep it on ice for detection.
- ⑤ Meanwhile, determine the protein concentration of supernatant (E-BC-K318-M).

Cell (adherent or suspension) samples:

- ① Harvest the number of cells needed for each assay (initial recommendation 1×10^6 cells).
- ② Wash cells with PBS (0.01 M, pH 7.4).
- ③ Homogenize 1×10^6 cells in 300-500 μ L PBS (0.01 M, pH 7.4) with a ultrasonic cell disruptor at 4°C.
- ④ Centrifuge at 10000 \times g for 10 min to remove insoluble material. Collect supernatant and keep it on ice for detection.
- ⑤ Meanwhile, determine the protein concentration of supernatant

(E-BC-K318-M).

② Dilution of sample

The recommended dilution factor for different samples is as follows (for reference only):

Sample type	Dilution factor
Human serum	1
Human urine	1-2
10% Rat liver tissue homogenate	1
10% <i>Epipremnum aureum</i> tissue homogenate	1
HepG2 cells	1
HepG2 cell culture supernatant	1

Note: The diluent is normal saline (0.9% NaCl) or PBS (0.01 M, pH 7.4). For the dilution of other sample types, please do pretest to confirm the dilution factor.

The key points of the assay

- ① The supernatant of sample preparation after centrifugation must be clarified, otherwise centrifuge again.
- ② After the sample reaction, ensure to complete the detection within 25 min.

Operating steps

1. For serum (plasma) and other liquid samples

- ① Sample tube: Add 100 μL of buffer solution to 1.5 mL EP tube.
Control tube: Add 100 μL of buffer solution to 1.5 mL EP tube.
- ② Sample tube: Add 10 μL of sample to the tube.
Control tube: Add nothing.
- ③ Add 200 μL of chromogenic working solution and 50 μL of ferric salt working solution to sample tube and control tube.
- ④ Mix well and incubate the tubes at 37°C for 30 min.
- ⑤ Add 10 μL of stop solution to sample tube and control tube.
- ⑥ Sample tube: Add nothing.
Control tube: Add 10 μL of sample to the tube.
- ⑦ Mix fully and stand for 5 min at room temperature. Take 300 μL of reaction liquid to 96 well microplate and measure the OD value of each well at 520 nm with microplate reader.

2. For tissue and cells samples

- ① Sample tube: Add 100 μL of buffer solution to 1.5 mL EP tube.
Control tube: Add 100 μL of buffer solution to 1.5 mL EP tube.
- ② Sample tube: Add 10 μL of sample to the tube.
Control tube: Add nothing.
- ③ Add 200 μL of chromogenic working solution and 50 μL of ferric salt working solution to sample tube and control tube.
- ④ Mix fully and incubate the tubes at 37°C for 30 min.
- ⑤ Add 20 μL of stop solution to sample tube and control tube.
- ⑥ Sample tube: Add nothing.
Control tube: Add 10 μL of sample to the tube.
- ⑦ Add 20 μL of clarificant to sample tube and control tube.

- ⑧ Mix fully and stand for 5 min at room temperature. Take 300 μL of reaction liquid to 96 well microplate and measure the OD value of each well at 520 nm with microplate reader.

3. For whole blood samples

- ① Sample tube: Add 100 μL of buffer solution to 1.5 mL EP tube.
Control tube: Add 100 μL of buffer solution to 1.5 mL EP tube.
- ② Sample tube: Add 10 μL of sample to the tube.
Control tube: Add nothing.
- ③ Add 200 μL of chromogenic working solution and 50 μL of ferric salt working solution to sample tube and control tube.
- ④ Mix fully and incubate the tubes at 37°C for 30 min.
- ⑤ Add 20 μL of stop solution to sample tube and control tube.
- ⑥ Sample tube: Add nothing.
Control tube: Add 10 μL of sample to the tube.
- ⑦ Mix fully and stand for 5 min at room temperature. Take 300 μL of reaction liquid to 96 well microplate and measure the OD value of each well at 520 nm with microplate reader.

Calculation

The sample:

1. Serum (plasma), whole blood and other liquid samples

Definition: At 37 °C, the OD value of the reaction system was increased 0.01 by 1 mL of sample per minute is defined as a unit of total antioxidant capacity.

$$\text{T-AOC activity (U/mL)} = \frac{\Delta A}{0.01} \div 30^* \times \frac{V_1}{V_2} \times f$$

2. Tissue and cell samples

Definition: At 37 °C, the OD value of the reaction system was increased 0.01 by 1 mg of protein per minute is defined as a unit of total antioxidant capacity.

$$\text{T-AOC activity (U/mgprot)} = \frac{\Delta A}{0.01} \div 30^* \times \frac{V_1}{V_2} \times f \div C_{pr}$$

[Note]

ΔA : $OD_{\text{Sample}} - OD_{\text{Control}}$

*: The reaction time, 30 min.

V_1 : The total volume of reaction, mL.

V_2 : The volume of sample added to the reaction, mL.

f: Dilution factor of sample before tested.

C_{pr} : Concentration of protein in sample, mgprot/mL.

Appendix I Performance Characteristics

1. Parameter:

Intra-assay Precision

Three human serum samples were assayed in replicates of 20 to determine precision within an assay. (CV = Coefficient of Variation)

Parameters	Sample 1	Sample 2	Sample 3
Mean (U/mL)	3.50	64.50	138.50
%CV	5.1	4.7	4.6

Inter-assay Precision

Three human serum samples were assayed 20 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean (U/mL)	3.50	64.50	138.50
%CV	5.3	5.7	5.8

Recovery

Take three samples of high concentration, middle concentration and low concentration to test the samples of each concentration for 6 times parallelly to get the average recovery rate of 96%.

	Standard 1	Standard 2	Standard 3
Expected Conc. (U/mL)	22.5	84.6	164.5
Observed Conc. (U/mL)	22.3	80.4	154.6
Recovery rate (%)	99	95	94

Sensitivity

The analytical sensitivity of the assay is 0.62 U/mL. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

Appendix Π Example Analysis


Example analysis:

Take 10 µL of human serum sample and carry the assay according to the operation steps. The results are as follows:

The average OD value of the sample is 0.081, the average OD value of the control is 0.020, and the calculation result is:

$$\text{T-AOC (U/mL)} = \frac{0.081 - 0.020}{0.01} \div 30 \times \frac{0.37}{0.01} = 7.52 \text{ U/mL}$$

Detect human serum, 10% rat liver tissue homogenate (the concentration of protein in sample is 13.99 mgprot/mL), 10% Epipremnum aureum tissue homogenate (the concentration of protein in sample is 1.59 mgprot/mL) and HepG2 cells (the concentration of protein in sample is 5.02 mgprot/mL) according to the protocol, the result is as follows:

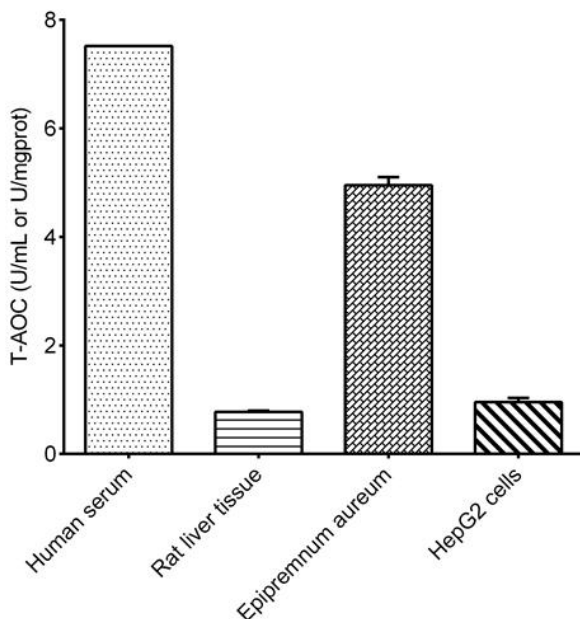

Appendix III Publications

1. Hou B , Wang D , Yan F ,et al.Fhb7-GST catalyzed glutathionylation effectively detoxifies the trichothecene family[J].Food Chemistry, 2024(May 1):439.DOI:10.1016/j.foodchem.2023.138057.
2. Nebrisi E E .Phytochemical Evaluation of *Lepidium meyenii*, *Trigonella foenum-graecum*, *Spirulina platensis*, and *Tribulus arabica*, and Their Potential Effect on Monosodium Glutamate Induced Male Reproductive Dysfunction in Adult Wistar Rats[J].Antioxidants, 2024, 13.DOI:10.3390/antiox13080939.
3. Bao L , Huang Y , Gu F ,et al.Zearalenone induces liver injury in mice through ferroptosis pathway[J].The Science of the total environment, 952:175875[2025-03-03].DOI:10.1016/j.scitotenv.2024.175875.
4. Marhamati S , Younesian O , Mir S M ,et al.The effects of high doses of selenium supplementation on mRNA and protein levels of cMLCK levels and total antioxidant capacity in rat heart tissue[J].Food and Chemical Toxicology, 2024, 191(000):4.DOI:10.1016/j.fct.2024.114886.
5. Obeid R A , Mohammed R A , Kaskoos R A ,et al.Exploring the antioxidant potential of *Moringa oleifera* leaf extracts mitigating doxorubicin-induced cardiotoxicity in male rats[J].Journal of Advanced Pharmaceutical Technology & Research, 2024, 15(3):166-170.DOI:10.4103/JAPTR.JAPTR_531_23.

Statement

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.

